



EDQM SYMPOSIUM ON MICROBIOLOGY

10-11 October 2017

EDQM, Strasbourg, France

Poster Presentations

How to validate challenging parameters of a quantitative rapid method in Pharma Industry? Two Customer Examples



Vincent Beguin, Millipore S.A.S, France
Anke Hossfeld, Merck KGaA, Darmstadt, Germany
Prof. Dr. Edwin van den Heuvel, Eindhoven University of Technology, Netherlands


Introduction

The interest of Pharmaceutical Industry to implement methods which allow faster results and release of their products is very high. For the majority of customers the validation of Rapid Microbiological Methods (RMM) according to EP 5.1.6 is still challenging. Especially the parameters that require advanced statistical knowledge like accuracy, precision and linearity could prevent customers from completing their validation and using of the method in routine. Additionally validation work can take a lot of resources.

The following customer examples of global Pharmaceutical companies provide two different approaches how to implement and validate a RMM method for the application of Rapid Bioburden Testing.

Both studies were performed with the Milliflex® Quantum, a fluorescence-based technology for filterable samples.

The principle of the fluorescence detection is based on an enzymatic reaction. The fluorogenic substrate used is a non-fluorescent viability marker that is cleaved by nonspecific intracellular enzymes resulting in a fluorescent product [1]. Accumulation of fluorescence inside cells is an indicator of microbial metabolism activity and membrane integrity. The dye is diluted in a staining buffer allowing cell membrane permeabilization and thus passive dye introduction into cells, maintaining the cells viability.

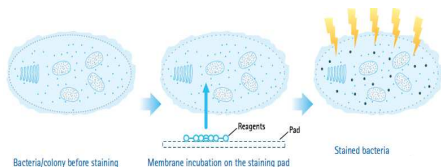

Validation Principles

Milliflex® Quantum method is validated as an alternative method to the compendial test of bioburden for pharmaceutical products (Microbiological examination of Non Sterile Products, EP 2.6.12, USP <61> or JP 4.05) according to Guidelines EP 5.1.6, USP <1223> and PDA TR 33, Validation of Alternative Microbiological Methods [5], [6], [7], [8].

We consider here the Performance Qualification done by the user, considering that a primary validation has been carried out by the supplier (EP 5.1.6 gives a very comprehensive matrix with the respective rules of Supplier and User in the validation process)

As Milliflex Quantum is a quantitative method, the validation of a Rapid Microbiological Method comprises the following parameters:

- LOQ/LOD
- Precision
- Linearity/ range
- Specificity
- Robustness/ Ruggedness
- Suitability
- Equivalence

Methodology

To perform the validation experiments, the alternative method (Milliflex® Quantum) is compared to the traditional method by membrane filtration (Milliflex®), using materials and equipment provided by the supplier. As the method is to be validated for its intended use, to demonstrate the specificity of the method, experiments were done with culture collection strains (ATCC) but also in-house isolates, some of which had been stressed (heat or starvation). Validation studies require statistics because they include experiments which provide data that must be analyzed and interpreted. In particular, quantal tests related to the sensitivity of the method (LOQ/ LOD), precision and accuracy require a good level of statistical knowledge and methods. Then, we focus on these parameters because they are considered as challenging for customers and, additionally, specificity is also treated, because it is key for the performance and justify the choice of an alternative method.

In both customer cases, Milliflex® Quantum is validated as an alternative global bioburden method with a reduced incubation time of 72 H instead of 5-7 days. In customer case 1 the Milliflex® Quantum is used as a qualitative test for LOD (using MPN) and as a quantitative test for Specificity.

Merck and the M logo are trademarks of Merck KGaA, Darmstadt, Germany. Milliflex is a registered trademark of Merck KGaA, Darmstadt, Germany. Bioball® is a registered trademark of Biooneuro. © 2016 Merck KGaA, Darmstadt, Germany. All rights reserved.


Validation Parameters and Statistical Methods

customer 1 [2]

Limit of Detection and (Quantification)

LOD and LOQ are the lowest number of microorganisms that can be respectively detected or accurately counted. LOQ was not in the scope as counting of colonies are done by an operator in both cases.

Test by MPN: inoculation of rinsing solution with 50, 5, 0.5 and 0.05 CFU. Alternative method (RBB) and compendial one (TBB) tested in parallel, two runs of each 10 replicates per concentration and microorganism (15 microorganisms including 7 in-house isolates). See results on Fig. 1.

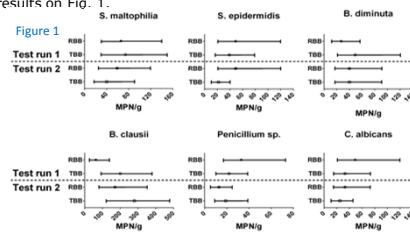

Specificity

The specificity of a method is defined as the potential to detect a broad range of microorganisms.

Remark: False positive rate is also to be tested, with a great number of blank test repetitions.

In this example, the specificity is demonstrated with 15 microorganisms including 7 representative stressed in-house isolates.

Test: 2 test runs of 10-100 CFU in 100mL with 3 replicates per microorganism. For some strains, the sample size is increased to reach the required test power. The CFU count for alternative test should not be statistically different as compared to the compendial test. For each run a 2-sample t-test at a confidence level of 95% is performed. (p-value must be >0.05). Finally, a limit power calculation is used to demonstrate non inferiority, with a test of ≥ 0.8 . See results Table 1.

| Species | Sample Size | RBB mean +/- SD (CFU) | TBB mean +/- SD (CFU) | p-value | Test Power |
|-------------------------------------|-------------|-----------------------|-----------------------|---------|------------|
| <i>Pseudomonas aeruginosa</i> | 5/5 | 33 +/- 3 | 40 +/- 7 | 0.26 | 0.99 |
| <i>Staphylococcus aureus</i> | 5/5 | 53 +/- 4 | 50 +/- 6 | 0.45 | 1.00 |
| <i>Bacillus subtilis</i> | 8/9 | 36 +/- 4 | 45 +/- 4 | 0.00 | 1.00 |
| <i>Escherichia coli</i> | 9/9 | 23 +/- 5 | 20 +/- 4 | 0.25 | 0.93 |
| <i>Burkholderia cepacia</i> | 6/5 | 75 +/- 12 | 72 +/- 7 | 0.53 | 0.99 |
| <i>Stenotrophomonas maltophilia</i> | 6/5 | 33 +/- 7 | 31 +/- 5 | 0.59 | 0.82 |
| <i>Bacillus licheniformis</i> | 6/5 | 21 +/- 2 | 22 +/- 3 | 0.51 | 0.87 |
| <i>Bacillus clausii</i> | 9/9 | 54 +/- 10 | 53 +/- 8 | 0.87 | 0.79 |
| <i>Staphylococcus epidermidis</i> | 5/5 | 33 +/- 3 | 33 +/- 5 | 0.92 | 0.93 |
| <i>Staphylococcus warneri</i> | 9/9 | 38 +/- 9 | 37 +/- 9 | 0.80 | 0.87 |
| <i>Pseudomonas citrea</i> | 6/5 | 46 +/- 7 | 41 +/- 5 | 0.11 | 0.95 |
| <i>Aspergillus niger</i> | 6/5 | 79 +/- 7 | 77 +/- 3 | 0.64 | 1.00 |
| <i>Penicillium sp.</i> | 6/5 | 88 +/- 12 | 90 +/- 5 | 0.72 | 1.00 |
| <i>Aspergillus brasiliensis</i> | 6/5 | 46 +/- 7 | 48 +/- 2 | 0.52 | 0.89 |
| <i>Candida albicans</i> | 9/9 | 52 +/- 7 | 55 +/- 3 | 0.45 | 0.96 |

customer 2

Accuracy and linearity

Note: *Staphylococcus aureus* (ATCC 6538) is treated as an example but each microorganism from culture collections and isolates can be tested by the same methodology.

Test: a stock solution (Vt) is spiked with 8 BioBall® of 550 CFUs (4400 CFU), 4 dilutions are created from Vt with volumes: V1=36 mL, V2=32.4 mL, V3=18 mL, V4=0.72mL

Each volume is complemented to 36 mL and then fully tested with Rapid method (RMM) and Compendial (CM) i.e., 18 X1 mL for each.

- To demonstrate accuracy, the total number of observed CFU are pooled over all dilutions for each method separately (X_{RMM} and X_{CM}) and the likelihood ratio test is calculated:

$$LRT = 2[\ln(X_{RMM}) - \ln(X_{RMM} + X_{CM}/2)] + X_{CM}[\ln(X_{RMM} + X_{CM}/2)]$$

LRT larger than 3,841 indicates a difference in detection. See results in Table 2. [3],[4]

- To demonstrate the linearity A regression curve is established for each method separately with Expected versus Observed counts on dilution (See Figure 2). Expected counts are derived from the total counts (X_{RMM} and X_{CM}) proportionally to the dilution volumes. Linearity is obtained when the regression line does not deviate from the line $y=x$.

Precision

Candida albicans (ATCC 10231) is treated as an example but each microorganism from culture collections and isolates can be tested by the same methodology.

Test: create a low and high spiked dilution over multiple days that is analyzed by multiple analysts (8 runs of 4 samples for each method). Calculate Repeatability (%) and Intermediate Precision (%) via a random effects ANOVA model (see ICH Q2(R1)). Results in Table 3 & Table 4. [3]

Discussion of Results


Limit of Detection

As demonstrated in Fig. 1, in all cases the 95% confidence intervals of the traditional and the rapid bioburden test do overlap, no significant difference regarding the LOD of any of the test strains is observed demonstrating adequate LOD for the alternative method.

Specificity

As we can see in Table 1, after exclusion of some outliers¹ with the Grubb's test, the specificity is fully demonstrated for 14 stains. For *Bacillus subtilis*, the Rapid method is tested against the Traditional one by a non-inferiority test at a confidence level of 95% with a boundary of 70%. (EP 2.6.12 and USP <1227> showing that the difference is acceptable.

| Dilution | Dilution V1 | | Dilution V2 | | Dilution V3 | | Dilution V4 | |
|----------|-------------|----|-------------|----|-------------|----|-------------|----|
| | AL | CM | AL | CM | AL | CM | AL | CM |
| 31 | 17 | 30 | 50 | 26 | 25 | 3 | 1 | |
| 47 | 47 | 38 | 40 | 70 | 35 | 1 | 2 | |
| 36 | 47 | 25 | 45 | 10 | 33 | 1 | 1 | |
| 15 | 40 | 41 | 35 | 27 | 14 | 1 | 0 | |
| 12 | 37 | 33 | 42 | 24 | 11 | 0 | 0 | |
| 37 | 45 | 10 | 10 | 24 | 25 | 1 | 1 | |
| 16 | 16 | 32 | 41 | 29 | 26 | 2 | 0 | |
| 21 | 42 | 34 | 28 | 21 | 26 | 1 | 1 | |
| 38 | 46 | 21 | 18 | 15 | 16 | 2 | 0 | |
| 48 | 41 | 48 | 26 | 20 | 30 | 2 | 2 | |
| 21 | 40 | 10 | 44 | 20 | 29 | 1 | 0 | |
| 17 | 45 | 27 | 22 | 28 | 1 | 1 | 0 | |
| 21 | 52 | 10 | 11 | 20 | 26 | 1 | 0 | |
| 37 | 15 | 30 | 58 | 17 | 15 | 0 | 1 | |
| 41 | 45 | 29 | 32 | 28 | 31 | 1 | 1 | |
| 43 | 34 | 30 | 41 | 22 | 17 | 1 | 4 | |
| 47 | 40 | 41 | 40 | 30 | 15 | 0 | 1 | |
| 49 | 46 | 31 | 49 | 16 | 22 | 2 | 2 | |



Accuracy & linearity

After pooling total number of observed CFU for each method (Table 2), the Likelihood Ratio Test is calculated: $LRT=0,43 < 3,841$. In conclusion, no significant difference is observed between accuracy of both methods. For the linearity, further investigations on the regression curve and associated slopes demonstrate perfect linearities of both methods.

Precision

| Run | Compendial | | Milliflex Quantum | |
|-----|------------|-----------|-------------------|-----------|
| | V1 (36) | V2 (32.4) | V1 (36) | V2 (32.4) |
| 1 | 14.3 | 17.1 | 15.1 | 15.3 |
| 2 | 17.5 | 18.7 | 15.0 | 14.9 |
| 3 | 17.8 | 16.9 | 17.3 | 17.1 |
| 4 | 18.1 | 17.0 | 16.6 | 16.1 |
| 5 | 18.5 | 18.6 | 18.0 | 17.8 |
| 6 | 15.0 | 14.9 | 13.6 | 13.8 |
| 7 | 18.3 | 18.0 | 17.0 | 16.9 |
| 8 | 21.3 | 20.7 | 20.5 | 21.0 |


| Dilution | V1 (36) | | V2 (32.4) | |
|----------------------------|------------|-------------|------------|-------------|
| | Compendial | Alternative | Compendial | Alternative |
| Average | 17.75 | 18.25 | 17.47 | 18.41 |
| Repeatability (%) | 18.1 | 29.2 | 14.6 | 12.1 |
| Intermediate Precision (%) | 20.1 | 26.0 | 15.3 | 13.4 |

After calculation of repeatability and intermediate precision (see Table 4) with data available on Table 3, we demonstrate that, as CV-repeatability satisfies the criteria based on Poisson and the total variation is less than 30% for both methods, the precision is fully acceptable for the alternative method.

Summary

With the right validation set-up and statistical approach it can be demonstrated that RMM methods provide the same performance as traditional microbiological methods adding additional advantage like time-to-release to the routine testing. Moreover, the customer examples show that statistical requirements of the EP 5.1.6 chapter can be overcome through the use of relevant tools. However, resource and time for validation can be limited using statistical support or service offer from method suppliers.

References
[1] Baumstamler, A. et al. (2009). Milliflex® Quantum: A Fluorescence-based Platform for the Rapid Detection of Contaminants in Filterable Products (Poster).
[2] Gordon, O., Goverde, M., Staerk, A. et al. Validation of Milliflex Quantum for Bioburden Testing of Pharmaceutical Products. PDA J Pharm Sci and Tech 2017, 71 205-224.
[3] Van den Heuvel, ER, Ijerman-Boon PC. A comparison of Test Statistics for the Recovery of Rapid Growth-Based Enumeration Tests. Pharmaceutical Statistics, 2013 12(5): 291-299.
[4] Goverde, M., Van den Heuvel, ER, Live Webinar: Streamline your Rapid Microbiological Method Validation, 2016, May 17.
[5] U.S. Pharmacopoeial Convention, USP 40-NF 35, USP<61>, USP<1223>, USP<1210>.
[6] Council of Europe, EDQM, European Pharmacopoeia, Ph. Eur. 9.2, EP 2.6.12, EP 5.1.6.
[7] PMDA, Japanese Pharmacopoeia, JP 17th edition, 4.05.
[8] Parenteral Drug Association, PDA TR 33 (Rev 2013).

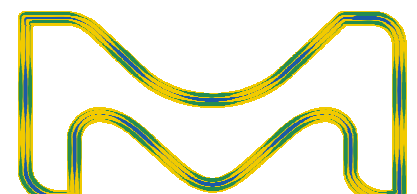

Evaluation of a Rapid Microbiological Method for filterable raw materials in Pharma Industry




Dr. Michael Rieth, Merck KGaA, Darmstadt, Germany
Jan Freitag, Friedrich-Schiller-University, Jena, Germany
Anke Hossfeld, Merck KGaA, Darmstadt, Germany

Introduction

The study was performed as part of a Microbiological Quality Control project dealing with rapid microbiological methods (RMM) at Merck Healthcare, a biopharmaceutical company focused on the areas of oncology, neurodegenerative diseases and endocrinology.

The Milliflex® Quantum System and Aim

The principle of fluorescence detection is based on an enzymatic reaction. The fluorogenic substrate used is a non-fluorescent viability marker that is cleaved by nonspecific intracellular enzymes, resulting in a fluorescent product [1]. The viability marker exhibits bright green fluorescence, which is measurable at wavelengths between 480 and 490 nm (Fig. 1) [2]. The dye is diluted in a staining buffer, allowing cell membrane permeabilization and, thus, dye introduction into cells [1] [3]. Accumulation of fluorescence inside cells indicates microbial metabolic activity and membrane integrity. The aim of the study was to validate the Milliflex® Quantum rapid microbiological method for the examination of filterable raw materials that are common in microbiological quality control in the pharmaceutical industry. The effects of raw materials on growth were also of particular interest.

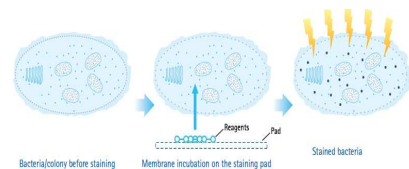


Materials & Methods

The causative microorganisms, *Staphylococcus aureus*, *Bacillus subtilis*, *Candida albicans* and *Aspergillus brasiliensis*, as well as the isolate, *Staphylococcus epidermidis*, were used for the validation. It was assumed that microorganisms, which are detected during microbiological quality control, would be stressed. This stress can occur through starvation, heat, dehydration or disinfectants. To simulate these conditions and induce spore formation, microorganisms were exposed to 60 °C (Fig. 2), or starvation in the case of *B. subtilis*. The target was to obtain an inoculum around 50 % compared to frozen stock solution [4]. Validation was achieved through one of two approved methods: inoculation during the last rinsing step, or direct inoculation of the raw material buffer solution. In the event of inhibition, the first method was used to obtain measurable results. Evaluation followed after three days. In parallel to the Milliflex® Quantum method, the traditional technique was performed with an incubation period of five days. Finally, the two methods were compared and assessed.


Discussion

Results & Prospects

As expected, the bacteria reacted sensitively to low pH, and their growth was inhibited, while the mold and yeast were mostly unaffected. Orange oil, peach aroma and orange aroma had the greatest inhibitory effect on all microorganisms except *A. brasiliensis*, which was only verifiably inhibited by orange aroma. The inhibition of the growth of *P. aeruginosa* and *B. subtilis* by sodium saccharin was expected at this concentration [5]. Nicotinamide had an inhibitory effect on *B. subtilis* and *P. aeruginosa*, but surprisingly not on *S. aureus* [6]. In comparison to the other organisms, stressed *B. subtilis* seemed to be highly sensitive to changes in pH and other conditions. In most cases, the Milliflex® Quantum System did not show significant differences in received values, since the statistical threshold was just one unit below 0.05. The high values in the recovery rates were due to the afore-mentioned inhibitory effects of the raw materials (Fig. 3, Orange oil). The low numbers of colony-forming units (CFU) also resulted in greater recovery rates. *A. brasiliensis* was not measurable after five days, thus determination of recovery rate and t-value were not feasible. However, evaluation via the Milliflex® Quantum System was possible.

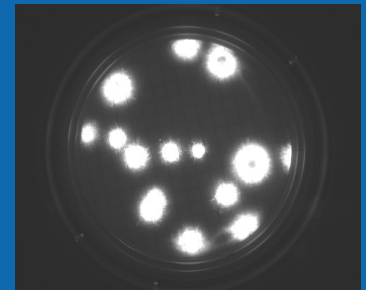

| Raw Materials | <i>A. brasiliensis</i> | | <i>C. albicans</i> | | <i>B. subtilis</i> | | <i>P. aeruginosa</i> | | <i>S. aureus</i> | | <i>S. epidermidis</i> | |
|--|------------------------|--------|--------------------|--------|--------------------|--------|----------------------|--------|-------------------|--------|-----------------------|--------|
| | Recovery Rate (%) | T-test | Recovery Rate (%) | T-test | Recovery Rate (%) | T-test | Recovery Rate (%) | T-test | Recovery Rate (%) | T-test | Recovery Rate (%) | T-test |
| Orange aroma | n.e. | n.e. | 100.00 | 0.87 | 94.83 | 0.74 | 92.94 | 0.20 | 73.66 | 0.34 | 100.00 | 1.00 |
| Ascorbic acid | n.e. | n.e. | 102.70 | 0.88 | 88.75 | 0.30 | 119.35 | 0.59 | 102.60 | 0.91 | 100.00 | 1.00 |
| Deoxyphenol | n.e. | n.e. | 92.41 | 0.10 | 100.00 | 1.00 | 79.37 | 0.06 | 113.11 | 0.07 | 117.07 | 0.31 |
| Hexaphenol | n.e. | n.e. | 96.67 | 0.56 | 87.01 | 0.52 | 86.11 | 0.19 | 89.28 | 0.39 | 100.00 | 1.00 |
| Glycerol 85% PHA Prod | n.e. | n.e. | 90.00 | 0.39 | 106.19 | 0.18 | 78.95 | 0.18 | 117.81 | 0.44 | 118.10 | 0.06 |
| Glycerol 85% PHA Prod | n.e. | n.e. | 122.89 | 0.19 | 119.10 | 0.26 | 80.32 | 0.10 | 86.72 | 0.40 | 103.57 | 0.88 |
| Glycine PHA Prod | n.e. | n.e. | 102.96 | 0.87 | 96.49 | 0.92 | 81.82 | 0.50 | 108.93 | 0.71 | 127.93 | 0.10 |
| Metformin hydrochloride/Magnesium stearate 0.5 % | n.e. | n.e. | 81.06 | 0.07 | 119.10 | 0.26 | 74.19 | 0.42 | 110.00 | 0.75 | 106.06 | 0.86 |
| Sodium dihydrogen phosphate dihydrate PHA Prod | n.e. | n.e. | 95.29 | 0.65 | 90.91 | 0.57 | 100.00 | 1.00 | 79.55 | 0.35 | 100.96 | 0.96 |
| Nicotinamide PHA Prod | n.e. | n.e. | 102.44 | 0.81 | 111.86 | 0.40 | 106.25 | 0.77 | 112.50 | 0.55 | 112.62 | 0.28 |
| Orange oil | 85.71 | 0.65 | 250.00 | 0.40 | 100.00 | 1.00 | 117.39 | 0.71 | 103.51 | 0.92 | 94.59 | 0.83 |
| Peach aroma 501.079C | n.e. | n.e. | 98.63 | 0.71 | 110.29 | 0.47 | n.e. | n.e. | 104.88 | 0.80 | 100.44 | 0.92 |
| Pyridoxine hydrochloride PHA Prod | n.e. | n.e. | 108.03 | 0.17 | 108.62 | 0.63 | 104.00 | 0.78 | 115.00 | 0.39 | 100.00 | 1.00 |
| Sodium saccharin | n.e. | n.e. | 101.65 | 0.92 | 89.47 | 0.72 | 107.14 | 0.83 | 80.00 | 0.09 | 107.69 | 0.53 |
| Thiamine chloride hydrochloride PHA Prod | n.e. | n.e. | 101.37 | 0.92 | 109.68 | 0.10 | 80.00 | 0.25 | 74.19 | 0.11 | 118.75 | 0.16 |
| Thiamine chloride hydrochloride PHA Prod | 83.33 | 0.88 | 95.71 | 0.67 | 101.56 | 0.92 | 77.78 | 0.23 | 90.91 | 0.59 | 113.25 | 0.45 |

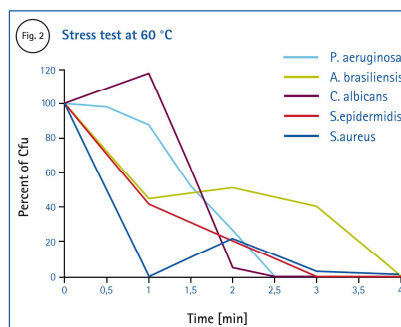


References

- [1] Baumstammier, A. et al. (2009). Milliflex® Quantum: A Fluorescence-based Platform for the Rapid Detection of Contaminants in Filterable Products (Poster).
- [2] Gordon, O., Gray, J., Anders, H., Staerk, A., and Schläel, O. (2011). Overview of rapid microbiological methods evaluated, validated and implemented for microbiological quality control. European Pharmaceutical Review, 16(2): 913.
- [3] Schlürer, J. and Rosswall, T. (1982). Fluorescein diacetate hydrolysis as a measure of total microbial activity in soil and litter. Applied and Environmental Microbiology, 43(6): 1256-1261.
- [4] Geall, N. and Rieth, M. (2012). Validation of rapid microbiological enumeration methods: A case study within its regulatory approach. Swiss Pharma, 34(6): 12-14.
- [5] Orlidzay, M. and Erdem, G. (2000). The Effect of Sodium Saccharin on the Growth of *Escherichia coli*, *Proteus*, *Pseudomonas aeruginosa*, *Staphylococcus epidermidis*, *Staphylococcus aureus* and *Enterococcus faecalis*. Turk Mikrobiyol Cem Derg., 30: 35-37.
- [6] Stretthoff, F. (1963). Inhibition of bacteria by 5-Fluorogenic acid and other analogues of nicotinic acid. Journal of Bacteriology, 85(1): 42-48.

Summary

The Milliflex® Quantum method represents a rapid alternative method for the quantification of contaminants in filterable products. The system has been successfully validated for three raw materials: glycerol, pyridoxine hydrochloride and thiamine chloride hydrochloride. This rapid microbiological method allows pharmaceutical manufacturers and quality control laboratories to address contamination events sooner, avoid line shutdowns, reduce storage costs and enable the earlier release of products to the market.

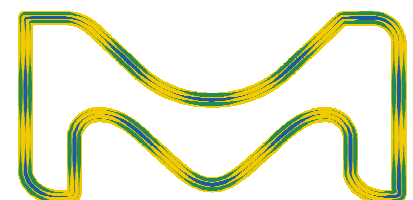

INTRODUCTION

Tight control of microbial environment surrounding health and personal care products is key for pharmaceutical industry. Quality and safety of final product is ensured through microbial monitoring of raw materials especially water, manufacturing environment and manufacturing process with in process and final product testing. Despite a number of benefits, alternative microbiology methods are poorly implemented and microbial controls are still performed using compendial petri dishes methods with operator-visual enumeration. These human-based tests are highly prone to individual mistakes (mis-labeling, mis-dilution, mis-counting, mis-reporting, loss of data ...) globally questioning the company data integrity policy. Here we present an innovative system, the EviSight™ compact, an integrated biomonitoring instrument able to incubate and read petri dishes in a real-time manner. This system is designed to be compliant with 21 CFR 11 requirements ensuring complete data integrity. The performances of the technology were challenged and demonstrated by 4 different and independent pharmaceutical industries through 3 main applications (90 mm and contact petri dish analysis, filter based analysis). Results obtained by these beta sites allow to establish statistically-relevant trueness, precision and equivalence of this method.

MATERIALS AND METHODS

• EVISIGHT™ COMPACT PRESENTATION

The EviSight™ Compact system is a smart incubator that automatically analyses commercial petri dishes for microbial detection and enumeration without colony staining or opening of the culture disposable.




Figure 1

Thanks to its interchangeable tray (figure 1), the EviSight™ Compact system can be used with a wide range of disposables: 90 mm / 55 mm / contact plates for filter-based (water and filterable products) and direct agar (environmental monitoring, product control ...) analysis.



Figure 2

With the first version, up to 4 readers can be stacked and connected to the same computer, offering greater incubation and processing capacity in a minimum of space (figure 2). Each reader can be run individually allowing disposable and set temperature (from 20 to 35°C) flexibility.

• STRAINS AND DISPOSABLES

Test microorganisms included in the study were sourced from culture collection and commercial calibrated strains.

- BioBall Multishot (bioMérieux):
Aspergillus brasiliensis ATCC 16404, ref. **56011**
Bacillus subtilis ATCC 6633, ref. **56012**
Candida albicans ATCC 10231, ref. **56013**
Pseudomonas aeruginosa ATCC 9027, ref. **56017**
Staphylococcus aureus ATCC 6538, ref. **56019**

- Culture collection:
Methylobacterium extorquens NBRC **15911**
Pseudomonas fluorescens NBRC **15842**
Additional in-house microorganisms from the different pharma industries collection.
The different disposables used are listed in the table 1:

| | PRODUCT | REFERENCE | SUPPLIER |
|------------------------------|---------------------------|--------------|------------|
| Culture media 90 mm | R2A | 43551 | bioMérieux |
| | TSA | 43011 | bioMérieux |
| | TSA 3P w. neutralizers | 43811 | bioMérieux |
| Culture media 55 mm | Sabouraud 3P | 43814 | bioMérieux |
| | R2A | AEB523487 | bioMérieux |
| Culture media Contact plates | Count-Tact 3P | 43691 | bioMérieux |
| | Count-Tact SDA 3P | 43812 | bioMérieux |
| White plain filters | Cellulose acetate filters | 11106-47-ACN | Sartorius |
| | PVDF filters | HVWP04756 | Millipore |
| | MicroFunnel filters | 516-8963 | Pall |

Table 1: Disposables used in the study

• EVISIGHT™ COMPACT EVALUATION

Filtration applications were tested using R2A plates with the 3 different filters spiked with 3 microorganism concentrations (5, 25 and 50 CFU/test), each condition tested in five replicates. 90 mm and contact plate applications were tested with direct inoculation of 3 microorganism concentrations (5, 25 and 50 CFU/test), each condition tested in five replicates. Incubation temperature were set according to pharmacopoeia. Maximum incubation times were set until optimal growth for easy detection by human eye.

• STATISTICAL ANALYSIS

EviSight™ compact performances were established from results obtained by four pharmaceutical industries using suitable statistical tests. EviSight™ compact enumeration was compared to operator-visual enumeration.

RESULTS AND DISCUSSION

• GROWTH KINETIC AND "GO BACK IN TIME" FEATURE

The EviSight™ compact system runs a high magnification technology enabling detection of microorganisms in their early stages of growth when they form microcolonies that are invisible to the naked eye (between 30 and 250 µm). As a real-time incubator and analyzer EviSight™ compact pictures the incubated plates every 30 minutes and powerful algorithms interpret microorganisms (micro)colonies growth. The system then deliver, for each plate incubated, a growth curve kinetic as illustrated in figure 3.

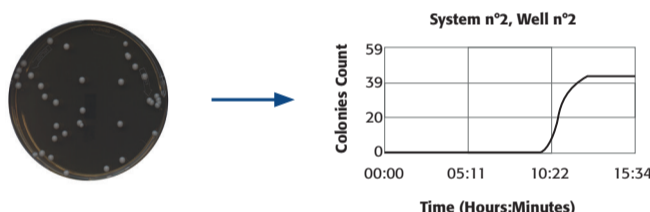


Figure 3: C. albicans growth curve

As the system record the successive images of each plate, it's possible to look microbial growth at different times of interest (before colonies swarming, pigmentation...). The figure 4 illustrates this "go back in time" feature for a swarming mold.

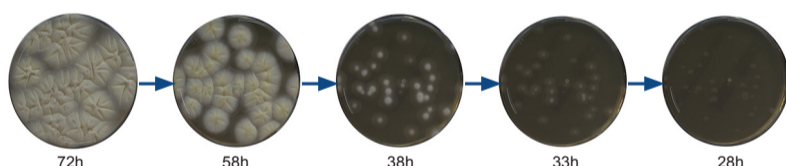


Figure 4: A. brasiliensis growth on contact plate monitored at different incubation times

• EVISIGHT™ COMPACT TRUENESS

The enumeration results from EviSight™ compact and manual were compared using a boxplot graphical representation (figure 5). This allows to visualize distribution characteristics of a quantitative variable.



Figure 5: Boxplots of microorganisms counts obtained with EviSight™ compact (left side of the pair) and manually (right side of the pair)

EviSight™ and manual methods show similar enumerations

• PRECISION

For both EviSight™ and manual enumeration, for each concentration level, repeatability is expressed through standard deviation and coefficient of variation (table 2). Statistical comparison of repeatability variances obtained with both enumeration methods was performed using the Fischer test (alpha = 5%) for each concentration level.

| Application | Target conc (CFU) | EviSight™ compact repeatability estimation | | | Manual Count repeatability estimation | | | p value | Fischer test Conclusion |
|----------------|-------------------|--|---------|--------|---------------------------------------|---------|--------|---------|---|
| | | Mean | std dev | CV (%) | Mean | std dev | CV (%) | | |
| 90 mm plates | 5 | 3.33 | 1.7 | 51.9% | 3.58 | 1.8 | 49.8% | 0.4278 | NO STATISTICALLY SIGNIFICANT DIFFERENCE |
| | 25 | 21.14 | 4.6 | 21.8% | 21.98 | 4.7 | 21.2% | 0.4703 | NO STATISTICALLY SIGNIFICANT DIFFERENCE |
| | 50 | 39.92 | 8.8 | 22.1% | 42.20 | 9.3 | 22.0% | 0.3683 | NO STATISTICALLY SIGNIFICANT DIFFERENCE |
| Contact plates | 5 | 3.28 | 1.9 | 57.8% | 3.23 | 1.9 | 58.6% | 0.5 | NO STATISTICALLY SIGNIFICANT DIFFERENCE |
| | 25 | 18.35 | 4.6 | 25.3% | 19.34 | 4.4 | 23.0% | 0.3451 | NO STATISTICALLY SIGNIFICANT DIFFERENCE |
| | 50 | 35.77 | 6.0 | 16.8% | 37.03 | 5.2 | 14.2% | 0.1005 | NO STATISTICALLY SIGNIFICANT DIFFERENCE |
| Filters | 5 | 4.86 | 2.9 | 60.2% | 4.42 | 2.7 | 60.9% | 0.2988 | NO STATISTICALLY SIGNIFICANT DIFFERENCE |
| | 25 | 21.07 | 5.1 | 24.3% | 20.69 | 5.1 | 24.5% | 0.4728 | NO STATISTICALLY SIGNIFICANT DIFFERENCE |
| | 50 | 44.73 | 7.4 | 16.4% | 44.05 | 6.9 | 15.7% | 0.3335 | NO STATISTICALLY SIGNIFICANT DIFFERENCE |

Table 2: Precision estimates and statistical comparison of EviSight™ compact and manual enumerations

Precision is demonstrated as all repeatability variances were shown to be statistically comparable between EviSight™ compact and manual enumeration.

• NUMERATION EQUIVALENCE OF EVISIGHT™ COMPACT AND MANUAL COUNTS.

Results obtained from EviSight™ compact and manual enumeration, for all concentration, were plotted together and a linear regression was performed (figure 6).

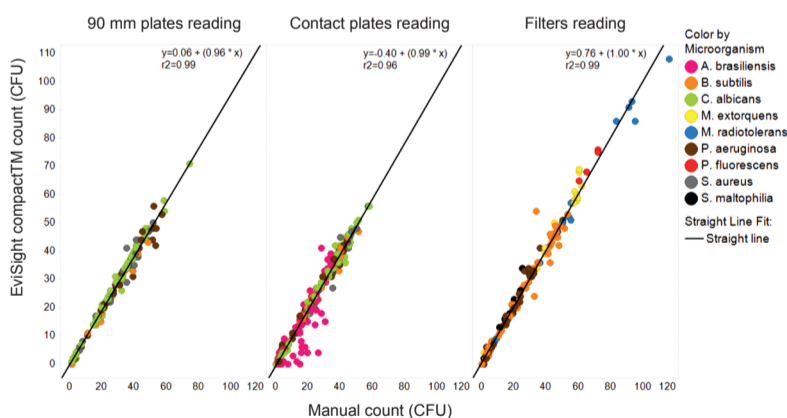


Figure 6 - Linear regression of EviSight™ enumeration results versus mean of manual plate counts

All regression analysis show a coefficient of determination r^2 greater than 0.9, a slope of the line of the best fit lying between 0.8 and 1.2 and a y-intercept close to zero. As there is no statistical difference of count between both methods, EviSight™ compact and manual enumerations are demonstrated equivalent.

CONCLUSIONS



Health and personal care products are closely reviewed by regulatory agencies as they involve patient / customer safety. In particular, microbial monitoring of raw materials, manufacturing environment and products is critical. Petri dishes traditional microbiology with operator-visual enumeration is still a reality in pharmaceutical industry but subject to human mistakes hard to justify. EviSight™ compact system provides you an automated analysis of your petri dishes and microbial enumeration in a real-time fashion. Performances of this system were demonstrated in terms of trueness, precision and equivalence to visual enumeration with in-house real-life pharmaceutical industry studies. Moreover, the real-time monitoring of microorganisms growth allow to generate growth curve and analyze previous images, a valuable tool for investigations.

REFERENCES

INTRODUCTION

R2A 3P[®] is a line extension of the existing 3P[®] product range. Therefore, this is an irradiated double wrap product, with flexible storage (2-25°C), extended shelf-life (6 months), and moisture/dehydration management. Based on R2A medium developed by Reasoner and Geldreich, R2A 3P[®] detects microorganisms that dwell in highly stressed environments, such as pharmaceutical water systems, and can be used for stressed microorganisms requiring low nutrient media for optimal growth.

The formulation and performance standards of R2A 3P[®] were designed to be compliant to the Pharmacopoeia recommendations [EP 9, JP 17, and USP 40] for R2A water testing. Additional regulatory guidance and peer-reviewed publications were referenced for product development and validation. The growth performance of the newly developed R2A 3P[®] was compared to commercially available media and included both Pharmacopoeia and environmental isolates. The EviSight™ Compact automated incubation and enumeration instrument uses high-magnification digital imaging technology for detecting colonies at early stages of growth (20-50 µm). Pictures are taken every 30 minutes. The system is designed to deliver data integrity and full traceability. This study evaluated R2A 3P[®] using the EviSight Compact and Pharmacopoeia isolates after standard filtration at minimum and maximum incubation times to determine feasibility for automated water testing.

MATERIALS AND METHODS

TESTED PRODUCTS

The R2A 3P[®] media developed at bioMérieux and other culture media used in this study are detailed in Table 1.

| bioMérieux Item No. | Name | Description |
|---------------------|---------------------|---|
| M1065 | R2A | Non-irradiated control |
| 421986 | R2A 3P [®] | Irradiated; 2-25°C storage; 6 month shelf-life |
| NA | Media A* | Irradiated; 2-8°C storage; 3.5 month shelf-life |
| NA | Media B* | Irradiated; 2-8°C storage; 4 month shelf-life |

Table 1: Culture Media used in this study

*Commercially available R2A media

LIBRARY OF TESTED MICROORGANISMS

A total of 70 microorganisms were used in this study and were sourced from commercially available and internal library collections and included wild isolates obtained from pharmaceutical manufacturers.

GROWTH PROMOTION TESTING

Growth promotion was evaluated with the panel of 70 strains. The microorganisms were prepared using a fresh cell suspension or BioBall[®] format. A target of <100 cells were used for all microorganisms. The cells were either applied directly to the test media using a spiral plater or were filtered through a 0.2 µm PES membrane. Performance testing was run in duplicate for both stressed (1 day at 2-8°C in sterile purified water) and non-stressed organism testing.

Plates were incubated at 30-35°C for USP/PE recommended and environmental organisms and at 20-25°C for JP recommended organisms for 3 to 7 days. Colony counts were performed using an automated colony counter. Acceptance criteria for microorganism recovery was between 50 – 200% compared to non-irradiated R2A controls.

EXUDATION

R2A 3P[®] was evaluated for condensation/exudation inside and outside the plate and packaging over the shelf-life of the product using the qualitative and quantitative scale outlined in Table 2.

Acceptance criteria was established to be ≤2 on the lid and ≤1 in the sleeve.

| Exudation score | Description |
|------------------|---|
| 0 – Dry | No fog, condensation or droplets |
| 1 – Condensation | Moist lid or with humidity area, no separate drops and/or droplets size < 1mm |
| 2 – droplets | Separate droplets size ≥ 1 mm, and ≤ 4 mm |
| 3 – Drops | Several big separate drops |
| 4 - Water | No separate drops, puddle of water in the lid |

Table 2: Exudation scale

DEHYDRATION

The newly developed R2A 3P[®] media was designed with a deeper fill volume (25 mL) to withstand extended incubation periods required for retrieval of stressed/slow growing organisms.

Dehydration was assessed over the shelf-life of the product using the scale shown in Table 3.

Acceptance criteria was established to be ≤10% of minor shrinkage/cracks of total samples tested.







| 1 - Fully Intact | 2 - Meniscus break | 3 - Retraction from side ≤2mm | 3 - Cracking ≤2mm | 4 - Retraction from side >2mm | 4 - Cracking >2mm |
|--|---|---|---|---|---|
|  |  |  |  |  |  |

Table 3: Dehydration scale

EVISIGHT™ COMPACT

Growth of Pharmacopoeia microorganisms (after standard filtration) on the EviSight Compact instrument (Figure 1) was evaluated at minimum and maximum incubation time on R2A 3P.

Two filter types were used to determine feasibility and included:

- Millipore™ - 0.45µm polyvinylidene fluoride (PVDF)
- Pall® - 0.2µm polyethersulfone (PES)



Figure 1: EviSight™ Compact Instrument, Single incubator

RESULTS AND DISCUSSION

GROWTH PERFORMANCE – STANDARD INOCULATION AND FILTRATION WITH STRESSED ORGANISMS

Growth promotion was evaluated on R2A 3P[®] and commercially available irradiated R2A culture media with a total of 70 microorganisms.

Growth promotion using membrane filtration was evaluated on R2A 3P[®] and commercially available irradiated R2A culture media with a total of 11 stressed microorganisms.

Figure 2 clearly illustrates R2A 3P[®] having better growth performance as compared to commercially available irradiated R2A media. R2A 3P[®] has the highest growth recovery rate without recorded failures for all microorganisms tested, whatever the inoculation method.

The growth promotion results for the Pharmacopoeia microorganisms (Table 4) show acceptable (50-200%) recovery for all tested media with R2A 3P[®] and Media B showing slightly better performance compared to Media A.

A total of 62 environmental isolates were tested for growth promotion. Only R2A 3P[®] was able to successfully support 100% recovery within acceptable limits. Table 5 details the isolates that R2A 3P[®] was able to detect compared to other commercially available R2A media. The results indicate the importance of including a wide-range of water and environmental microorganisms in product development.

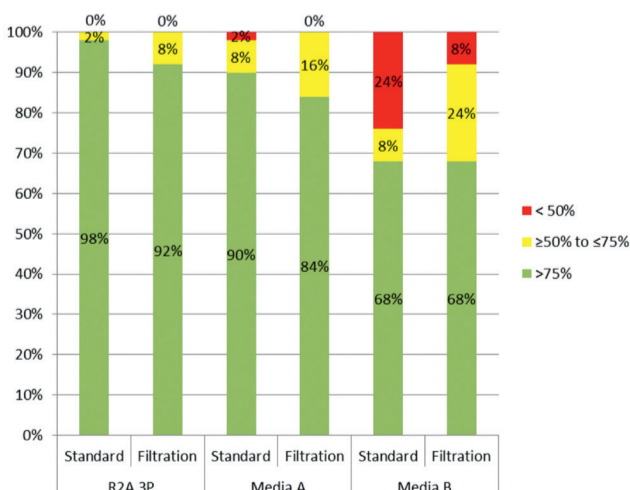


Figure 2: Growth performance consolidated recovery rate of R2A 3P[®] other irradiated R2A media, direct inoculation and Filtration with stressed organisms

RESULTS AND DISCUSSION CONTINUED

TESTED PRODUCTS

| Organisms | Temp °C | % Recovery Rate | | |
|--|---------|---------------------|---------|---------|
| | | R2A 3P [®] | Media A | Media B |
| % Recovery of Pharmacopoeia Organisms at 50-200% | | 100% | 100% | 100% |
| % Recovery of Pharmacopoeia Organisms at >75% | | 100% | 70% | 100% |

Table 4: Pharmacopoeia organism recovery, R2A 3P[®] vs. other irradiated R2A media

| Organisms | % Recovery Rate | | |
|---|---------------------|---------|---------|
| | R2A 3P [®] | Media A | Media B |
| <i>Aeromonas media</i> API 1212102 | 102 | 96 | 24 |
| <i>Aeromonas sobria</i> 201402043 | 106 | 94 | 42 |
| <i>Bacillus licheniformis</i> 201402030 | 154 | 88 | 27 |
| <i>Brevundimonas vesicularis</i> 201402044 | 110 | 113 | 0 |
| <i>Chryseobacterium daecheongense</i> API 1310029 | 76 | 93 | 0 |
| <i>Corynebacterium striatum</i> 201401014 | 148 | 55 | 39 |
| <i>Cupriavidus pauculus</i> API 1310032 | 86 | 82 | 42 |
| <i>Enterococcus faecium</i> 201402002 | 117 | 11 | 14 |
| <i>Iodobacter fluviatilis</i> API 0606196 | 117 | 110 | 0 |
| <i>Ralstonia insidiosa</i> API 0512080 | 107 | 104 | 0 |
| <i>Ralstonia pickettii</i> 201509004 | 145 | 106 | 0 |
| <i>Sphingomonas leidyi</i> API 1310041 | 152 | 131 | 0 |
| <i>Sphingomonas leidyi</i> API 1310044 | 162 | 112 | 0 |
| <i>Sphingomonas paucimobilis</i> 201310007 | 123 | 112 | 0 |
| <i>Virgibacillus pantothenicus</i> 201402040 | 84 | 82 | 1 |

Table 5: Environmental organism recovery at ≤50%, R2A 3P[®] vs. other irradiated R2A media

To further illustrate growth and recovery:

- Figure 3 is an example of an environmental isolate on control and tested media,

- Figure 4 shows equal or better performance of R2A 3P[®] compared to non-irradiated R2A control, with the filtration method.

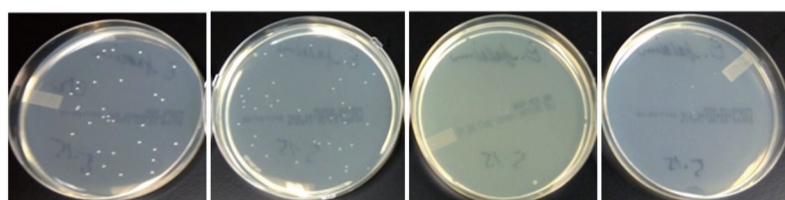


Figure 3: *Enterococcus faecium* 201402002 after 2 days incubation at 30-35°C

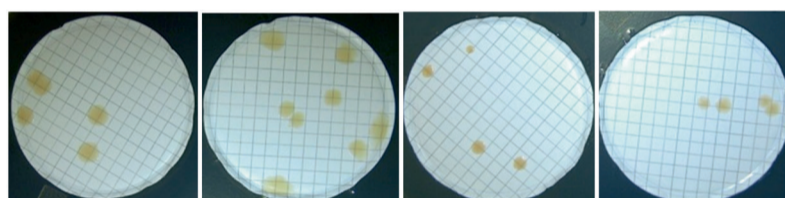


Figure 4: *Pseudomonas aeruginosa* ATCC 9027 after 3 days incubation at 30-35°C

EXUDATION

During stability shelf life testing, results from condensation/exudation monitoring show that R2A 3P[®] conforms to the required qualitative and quantitative scoring scale: ≤1 for sleeves and ≤2 for plate lids (Figure 5).


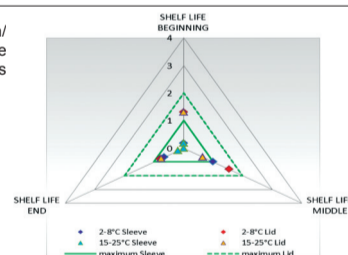


Figure 5: R2A 3P[®] exudation sleeve and plate lid scoring over shelf life

DEHYDRATION

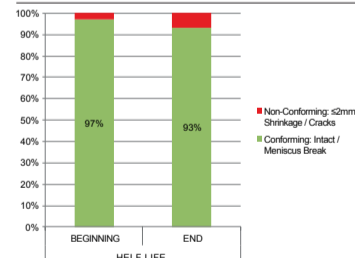

Stability testing for dehydration with extended incubation time during and up the end of total product shelf life show that R2A 3P[®] meets the required standards for optimal culture medium integrity at ≤10% of minor shrinkage/cracks of total samples tested (Figure 6).

Figure 6: Dehydration evaluation for R2A 3P[®] over shelf life

EVISIGHT™ COMPACT

The EviSight Compact feasibility testing with R2A 3P[®] show comparable results to manual reading using both PVDF and PES filter types (Table 6). The results using the 0.2 µm PES filter from Pall showed the least variation between minimum and maximum reading time points. The results support that R2A 3P[®] is compatible with EviSight™ Compact. Additional studies are being performed including mixed cultures to fully validate the media for automated water testing.

| Organism | Filter | Min / Max Incubation | Colony Forming Units | |
|---|-----------|----------------------|----------------------|----------|
| | | | Manual | EviSight |
| <i>Pseudomonas aeruginosa</i> ATCC 9027 | Millipore | 36 hours | 48 | 51 |
| | | 72 hours | 48 | 54 |
| | Pall | 36 hours | 48 | 40 |
| | | 72 hours | 48 | 45 |
| <i>Bacillus subtilis</i> ATCC 6633 | Millipore | 36 hours | 41 | 41 |
| | | 72 hours | 41 | 41 |
| | Pall | 36 hours | 38 | 36 |
| | | 72 hours | 38 | 36 |
| <i>Pseudomonas fluorescens</i> NBRC 15842 | Millipore | 72 hours | 65 | 64 |
| | | 5 days | 65 | 67 |
| | Pall | 72 hours | 27 | 27 |
| | | 5 days | 27 | 27 |
| <i>Methylobacterium extorquens</i> NBRC 15911 | Millipore | 5 days | 23 | 12 |
| | | 7 days | 28 | 28 |
| | | 5 days | 35 | 34 |
| | Pall | 7 days | 35 | 34 |
| | | 7 days | 35 | 34 |
| | | 7 days | 35 | 34 |

Table 6: EviSight™ Compact vs. manual enumeration results on R2A 3P[®] at minimum and maximum incubation

CONCLUSION

As a premium 3P[®] culture medium with flexible storage (2-25°C), R2A 3P[®] was carefully designed and developed for optimal performance with validation of consistent proven product performance up to the end of total shelf life (6 months).

The newly developed R2A 3P[®] showed equal or greater growth performance as compared to non-irradiated R2A and commercially available irradiated R2A media. R2A 3P[®] was the only tested medium able to successfully support growth recovery of 70 microorganisms. The results illustrate the importance of inclusion of environmental and stressed microorganisms during product development.

R2A 3P[®] is compatible with EviSight™ Compact allowing users to validate automated water testing with full data integrity and traceability.

Rapid Sterility Testing

Release your finished product in only 5 days under GMP

Key benefits of Rapid Sterility Test

- **RELEASE YOUR BATCH IN 5 DAYS**
– three times faster than the compendial method
- **SAVE STORAGE COSTS**
- **INCREASE THE QUALITY OF YOUR ANALYSIS**
– objective computer assisted reading
- **IDENTIFICATION OF CONTAMINATION POSSIBLE**
- **GUARANTEED GMP AND C-GMP CONDITIONS**

System validation and method validation

Method validation consists of different phases:


PQ 1: validation of the system without product matrix

PQ 2-1: suitability test on the product

PQ 2-2: comparability of both alternative and compendial methods on the product

Within PQ 1, criteria of Qualitative Method have been tested and proven to be compliant for each criterium.

Flow chart Rapid Sterility Test

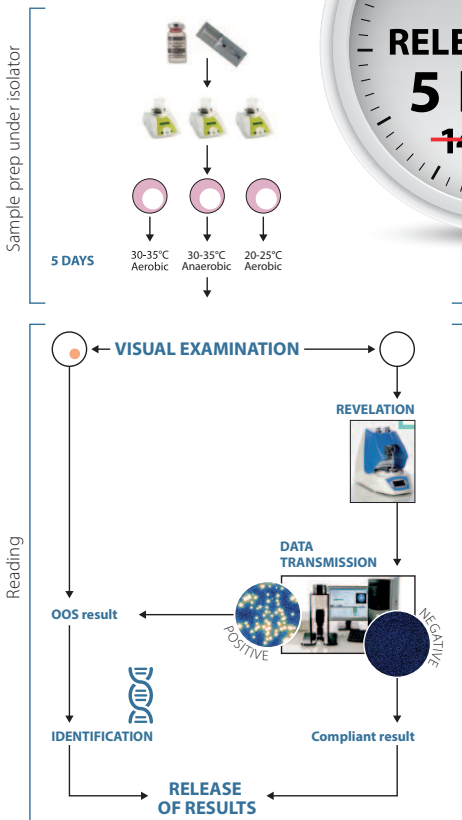

Validation results

Successful validation of PQ1 phase criteria

| CRITERIA | RESULT | STATUS |
|--------------------------|--|-------------|
| Specificity | Each microorganism was detected | Compliant ✓ |
| Accuracy | Equivalent to the compendial method | Compliant ✓ |
| Precision | Equivalent to the compendial method | Compliant ✓ |
| Robustness | Variations applied to the system had no impact | Compliant ✓ |
| Ruggedness | Variations applied to the system had no impact | Compliant ✓ |
| Limit of detection (LOD) | Equivalent to the compendial method, alternative method superior for Propioni-bacterium acnes and Micrococcus luteus | Compliant ✓ |

Validation results have proven that RST method is equivalent to the compendial method.

Why Confarma?

- 14 years of experience with sterility testing
- Experience with cell-therapy products
- Product specific validation
- Routine Testing
- Consulting
- Implementation support on your site
- Training

Regulations

- Ph. Eur. 5.1.6
- USP <1223>
- TR#33

Validation of a Rapid Sterility Test – Implementation Strategy and Perspective from a Contract Service Laboratory

C. Fromm, S. Gärtner, Dr. T. Meindl, Labor L+S AG, Germany



Abstract

Microbial contamination in sterile pharmaceutical manufacturing remains a great risk to patient safety. Thus, examination for sterility is often the final criterion for a batch approval. In line with the development of new, complex pharmaceuticals with short half life (ATMPs, proteins, etc.) the compendial 14-day test according to Ph. Eur. 2.6.1 and USP <71> is not appropriate. Thus, especially for these compounds, alternative rapid methods need to be implemented. The Development and use of these alternative methods is well supported by relevant authorities (e. g. PEI, FDA).

One of the most important prerequisites for approval is an appropriate validation of the alternative method, showing equivalence to the compendial test method.

Since there is no single technology suitable for any sample matrix, various technologies are available for various matrices. For samples not containing natural ATP, ATP bioluminescence measurement by means of Charles River's Celsis® AMPIScreen technology is well established. For samples containing ATP, a suitable established method can be BioMerieux BacTAlert® system which uses another ubiquitous cellular marker.

Goal of this project was to demonstrate the equivalence of an alternative, rapid method for sterility testing to the compendial, pharmacopoeial method on a broad spectrum of sample matrices. With this alternative methods, a broad spectrum of pharmaceuticals (and medical devices) can be tested for sterility fulfilling all requirements of the respective authorities and saving at least 50 % of time for test performance.

Validation Strategy

Well accepted validation requirements for alternative methods are described in:

- Ph. Eur. 5.1.6: Alternative methods for control of microbiological quality
- USP <1223>: Validation of Alternative Microbiological Methods
- PDA TR No 33: Evaluation, Validation and Implementation of Alternative and Rapid Microbiological Methods

Based on these sources a validation strategy was developed comprising of the following parameters:

| Parameter | Ph. Eur. 5.1.6 | USP <1223> | PDA TR no. 33 | Interpretation |
|--------------------------------|------------------------------|-----------------------|------------------------------|--|
| Specificity | yes | yes | yes | Detection and identification of all tested microorganisms |
| Detection limit | yes | yes | yes | Equivalence to the traditional method |
| Precision | yes | repeat precision | no | Precise results of the alternative method |
| Correctness | yes | no | no | Correct results of the alternative method |
| Robustness | yes | yes | yes | No influence of deliberately incorporated variations |
| Insensitivity | no | yes | yes | No influence of unavoidable variations |
| Equivalence or comparison test | yes (making use of products) | yes (without product) | yes (making use of products) | Equivalence to the traditional method with use of various products |

Results

Statistical backbone

Results were evaluated using a χ^2 strategy. The acceptance criterion was calculated to be $\chi^2 < 3.841$ (critical value for the 5 % significance level).

Detection Limit

The detection limit was determined by testing both methods in parallel. To reach statistical safety the following experiments have been performed (in total 720 independent experiments)

| Method | Number of positive results | Number of negative results | Total |
|--------------------|----------------------------|----------------------------|-------|
| Alternative method | 203 | 157 | 360 |
| Standard method | 199 | 161 | 360 |
| Total | 402 | 318 | 720 |

The calculated χ^2 value of 0.090 is < 3.841 ; thus, the acceptance criterion was fulfilled

Equivalence test

In the presence of various product matrices (parenteral solution, electrolyte solution, product to be dissolved, oily product, product containing dye) the equivalence of the compendial and the alternative method was tested.

Results:
Prerequisite method suitability test: no interferences such as falsely positive or falsely negative results were determined

Comparative results:

| Method | Number of positive results | Number of negative results | Total |
|--------------------|----------------------------|----------------------------|-------|
| Alternative method | 174 | 114 | 288 |
| Standard method | 174 | 114 | 288 |
| Total | 348 | 228 | 576 |

Calculated χ^2 value: 0.00 is < 3.841 , acceptance criterion was fulfilled.

Summary/conclusions

A straight forward validation strategy fulfilling international accepted regulatory requirements is suggested. A successful strategy in three steps was demonstrated:

1. General method validation without products (compare both methods); broad scale general equivalence study
2. Method suitability test using products (alternative method only); general system suitability test
3. Equivalence test using products (compare both methods); matrix specific validation, showing system suitable for a broad range of samples with different matrices

Greater than 1500 tests were needed to demonstrate the equivalence of the alternative and the compendial method. Since this broad scale approach of the study was performed, for any suitable matrix a compendial suitability test of the samples matrix has to be performed only. Thus, based on the preliminary work, a product specific implementation of the alternative method can be performed in the same time as for the compendial method.

Methods

In this project, an ATP bioluminescence technology (Charles River's Celsis® AMPIScreen) was performed. This method detects microbial derived ATP in the sample via an automated luciferin-luciferase enzyme reaction system. The underlying principle of the examination is in accordance to Ph. Eur. 2.6.1 and USP <71>, since membrane filtration and direct inoculation can be used. In the project, membrane filtration was performed. The only difference to the compendial evaluation by the human eye is an automated detection by means of ATP bioluminescence.

Membrane filtration

Process steps of classic membrane filtration based sterility testing (Ph. Eur. 2.6.1 and USP <71>):

1. Product filtration
2. Transfer of incubation media, followed by incubation
3. Visual examination after 14 days



Examination

Replacement of visual inspection by two technicians by automated, audit trail controlled examination.

Compendial method

14 days



Macroscopic evidence of microbial growth


Alternative method

7 days



Measurement of luminescence

Principle of AMPIScreen Technology:

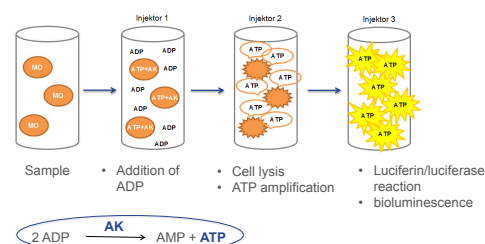

Literature

- United States Pharmacopoeial Convention. USP: Chapter <71> (2015) Sterility Tests.
- European Directorate for the Quality of Medicines & Health Care. Pharmeuropa: Ph.Eur.Chapter 2.6.1(2014) Sterility.
- European Directorate for the Quality of Medicines & Health Care. Pharmeuropa: Ph.Eur.Chapter 5.1.6 (2014) Alternative Methods for Control of Microbiological Quality.
- United States Pharmacopoeial Convention. USP: Chapter <1223> (2015) Validation of alternative microbiological methods.
- Parenteral Drug Association PDA (2013) Evaluation, Validation and Implementation of Alternative and Rapid Microbiological Methods. Technical Report No.33 (Revised2013).
- European Directorate for the Quality of Medicines & Health Care. Pharmeuropa: Ph. Eur. Chapter 5.1.9 (2014) Guidelines for using the test for sterility.

Contacts/Information



Stefan Gärtner
Head of Department for Rapid and Alternative Methods
Fon: +49(0)9708/9100-411
E-mail: stefan.gaertner@labor-ls.de



Carolin Fromm
Research & Development
Fon: +49(0)9708/9100-754
E-mail: carolin.fromm@labor-ls.de



Dr. Thomas Meindl
Division Manager
Fon: +49(0)9708/9100-750
E-mail: thomas.meindl@labor-ls.de